



EC Type Examination Certificate Number: **0120/ SGS0046**

# **Elster Metering Systems**

Tollgate Business Park  
Beaconside  
Stafford  
ST16 3HS

Instrument Identification:  
**A100C**

**Single Phase, Direct Connected, Credit, Import/Export, Active, Electricity Meter**

Instrument Traceable Number  
**0120/ SGS0046**

has been assessed and certified as meeting the requirements of

## **EC Directive 2004/22/EC** on Measuring Instruments Annex B

It is certified that the manufacturer's technical design and specimen for the above instrument has been examined and, based on the evidence submitted, it is considered that the instrument conforms to the requirements of MI-003 of EC Directive 2004/22/EC

This certificate must be used in conjunction with a certificate covering the product verification as required in Annex D or Annex F.

This certificate is valid for 10 years from 30th October 2009 until 29th October  
2019  
Issue 5

Certification is based on report number(s)  
Report 129970 dated 22nd October 2009  
Report 137550 dated 24th September 2010  
Report 150370 dated 17th August 2011

Authorised Signature

Jan Saunders

SGS United Kingdom Limited, Notified Body 0120  
Unit 202B Worle Parkway, Weston-super-Mare, BS22 6WA UK  
t +44 (0)1934 522917 f +44 (0)1934 522137 [www.sgs.com](http://www.sgs.com)

Contact Address  
SGS United Kingdom Ltd, Unit 10, South Industrial Estate, Bowburn, Durham, DH6 5AD UK  
t +44 (0)191 377 2000 f +44 (0)191 377 2020 [www.sgs.com](http://www.sgs.com)


<b>SGS</b>	EC-Type Examination Certificate Number: <b>0120/ SGS0046</b>	
	Issue Number: 5	Dated: 17 <sup>th</sup> May 2012

## 1. Technical Data

<b>Manufacturer</b>	Elster Metering Systems
<b>Meter Type</b>	A100C
<b>Voltage Rating (Un)</b>	220-250V
<b>Current Rating (Imin – Iref (Imax))</b>	<u>DIN Terminal Variant</u> 0,25-5(85)A 0,5-10(85)A (Any value Iref ≥ 5, up to Imax) <u>BS Terminal Variant</u> 0,25-5(100)A (Any value Iref ≥ 5, up to Imax)
<b>Frequency (Fn)</b>	50Hz
<b>Active Accuracy Class (kWh)</b>	A or B (kWh)
<b>Type of circuit</b>	1p2w
<b>Temperature Range</b>	DIN Variant -40°C to +60°C BS Variant -25°C to +55°C
<b>Software/ Firmware Version No Identification Location</b>	2-01167-F Nameplate
<b>Bill Of Materials Number</b>	JG0519 Sheets 2,3,4,4a,5,6,7,8,9
<b>IP Rating</b>	IP51
<b>Insulation Protective Class</b>	Class II
<b>LED Pulse Constant</b>	1000 imp/ kWh
<b>Impulse Voltage Rating</b>	6kV
<b>AC Voltage Rating</b>	4kV
<b>Main Cover Sealing Type</b>	Sealed for life
<b>Integrity of meter</b>	Inaccessible without breaking seals
<b>Intended Location of the Meter</b>	Indoor
<b>Type of Register</b>	LCD
<b>Terminal Arrangement(s)</b>	BS or DIN

<b>SGS</b>	EC-Type Examination Certificate Number:	
<b>0120/ SGS0046</b>		
Issue Number: 5	Dated: 17 <sup>th</sup> May 2012	

## 2. Photograph of Meter and Sealing Plan

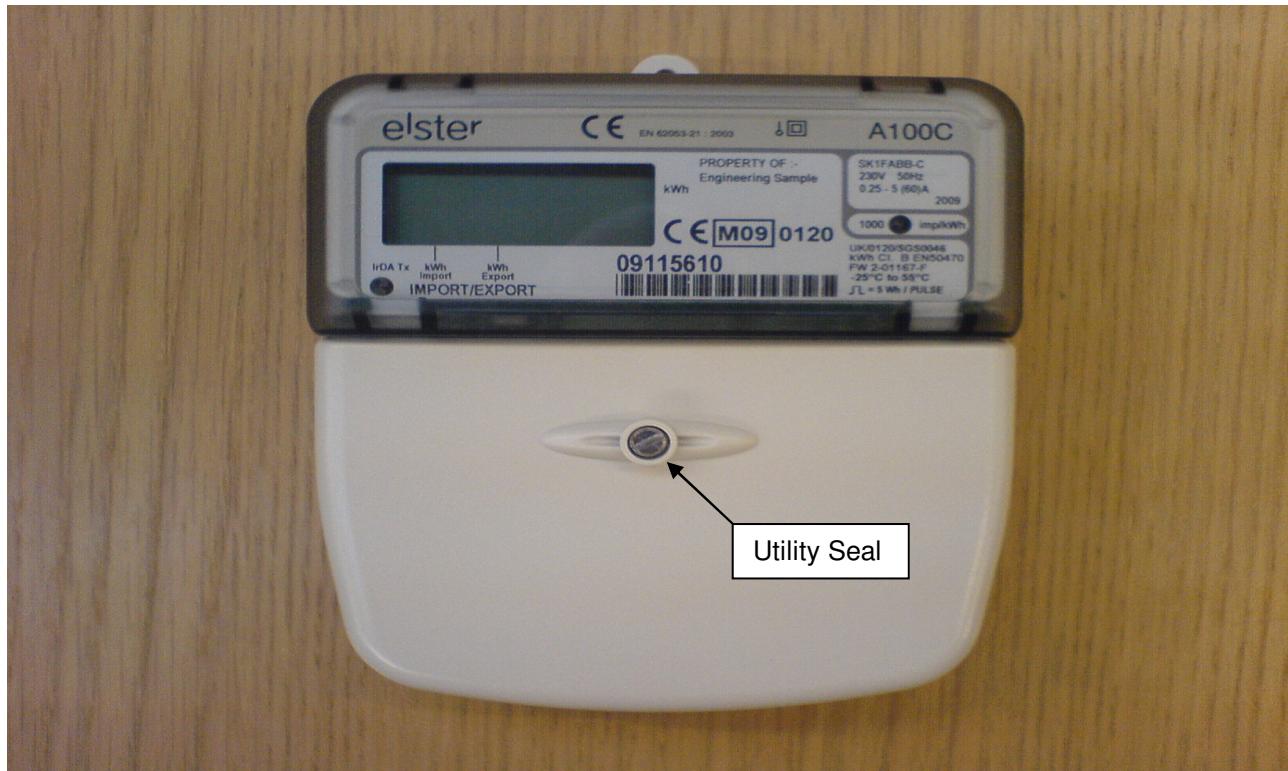

<b>SGS</b>	EC-Type Examination Certificate Number: <b>0120/ SGS0046</b>		
	Issue Number: 5		Dated: 17 <sup>th</sup> May 2012

### 3. Calculation of the composite error/ MPE

In addition to the accuracy requirements the composite error  $e_c$  of the meter is shown below

The composite error at a certain load is calculated from the following formula:

$$e_c = \sqrt{e^2(I.\cos\theta) + e^2(T.I.\cos\theta) + e^2(U.I.\cos\theta) + e^2(f.I.\cos\theta)}$$

where

$e^2(I.\cos\theta)$	=	Intrinsic error of meter at a certain load
$e^2(T.I.\cos\theta)$	=	Additional error due to variation of the temperature at the same load
$e^2(U.I.\cos\theta)$	=	Additional error due to variation of the voltage at the same load
$e^2(f.I.\cos\theta)$	=	Additional error due to variation of the frequency at the same load

Ambient Temperature Range 5 to 30 Degrees C						
Current	PF Cos	e(Icos)	e(TIcos)	e(UCos)	e(ficos)	%MPE
Imin	1.0	-0.10	0.33	0.13	0.05	<b>0.37</b>
Itr	1.0	-0.05	0.29	0.16	0.11	<b>0.35</b>
10ltr	1.0	0.14	0.19	-0.26	-0.29	<b>0.46</b>
Imax	1.0	0.14	0.34	-0.12	-0.09	<b>0.40</b>
Itr	0.5ind	-0.12	0.27	0.14	0.24	<b>0.41</b>
10ltr	0.5ind	0.16	0.19	-0.34	-0.27	<b>0.50</b>
Imax	0.5ind	0.11	-0.17	-0.20	-0.11	<b>0.31</b>
Itr	0.8cap	-0.17	-0.31	0.17	0.16	<b>0.42</b>
10ltr	0.8cap	0.17	0.32	-0.35	-0.29	<b>0.58</b>
Imax	0.8cap	0.01	0.19	-0.19	-0.13	<b>0.30</b>

Ambient Temperature Range -10 to 40 Degrees C						
Current	PF Cos	e(Icos)	e(TIcos)	e(UCos)	e(ficos)	%MPE
Imin	1.0	-0.10	0.67	0.13	0.05	<b>0.69</b>
Itr	1.0	-0.05	0.49	0.16	0.11	<b>0.53</b>
10ltr	1.0	0.14	0.52	-0.26	-0.29	<b>0.66</b>
Imax	1.0	0.14	-0.14	-0.12	-0.09	<b>0.25</b>
Itr	0.5ind	-0.12	0.66	0.14	0.24	<b>0.73</b>
10ltr	0.5ind	0.16	0.52	-0.34	-0.27	<b>0.70</b>
Imax	0.5ind	0.11	0.46	-0.20	-0.11	<b>0.53</b>
Itr	0.8cap	-0.17	0.53	0.17	0.16	<b>0.60</b>
10ltr	0.8cap	0.17	0.61	-0.35	-0.29	<b>0.78</b>
Imax	0.8cap	0.01	0.34	-0.19	-0.13	<b>0.41</b>

<b>SGS</b>	EC-Type Examination Certificate Number:					
	<b>0120/ SGS0046</b>					
	Issue Number: 5				Dated: 17 <sup>th</sup> May 2012	

Ambient Temperature Range -25 to 55 Degrees C						
Current	PF Cos	e(Icos)	e(TIcos)	e(UIcos)	e(fIcos)	%MPE
Imin	1.0	-0.10	0.86	0.13	0.05	<b>0.88</b>
Itr	1.0	-0.05	0.90	0.16	0.11	<b>0.92</b>
10ltr	1.0	0.14	0.82	-0.26	-0.29	<b>0.92</b>
Imax	1.0	0.14	-0.30	-0.12	-0.09	<b>0.36</b>
Itr	0.5ind	-0.12	0.78	0.14	0.24	<b>0.84</b>
10ltr	0.5ind	0.16	0.83	-0.34	-0.27	<b>0.95</b>
Imax	0.5ind	0.11	-1.00	-0.20	-0.11	<b>1.03</b>
Itr	0.8cap	-0.17	0.64	0.17	0.16	<b>0.70</b>
10ltr	0.8cap	0.17	0.90	-0.35	-0.29	<b>1.02</b>
Imax	0.8cap	0.01	-0.47	-0.19	-0.13	<b>0.52</b>

Ambient Temperature Range -40 to 70 Degrees C (OUTDOOR ONLY)						
Current	PF Cos	e(Icos)	e(TIcos)	e(UIcos)	e(fIcos)	%MPE
Imin	1.0	-0.10	1.24	0.13	0.05	<b>1.25</b>
Itr	1.0	-0.05	1.09	0.16	0.11	<b>1.11</b>
10ltr	1.0	0.14	1.14	-0.26	-0.29	<b>1.21</b>
Imax	1.0	0.14	-2.29	-0.12	-0.09	<b>2.30</b>
Itr	0.5ind	-0.12	0.85	0.14	0.24	<b>0.90</b>
10ltr	0.5ind	0.16	0.99	-0.34	-0.27	<b>1.09</b>
Imax	0.5ind	0.11	-1.98	-0.20	-0.11	<b>2.00</b>
Itr	0.8cap	-0.17	1.18	0.17	0.16	<b>1.21</b>
10ltr	0.8cap	0.17	1.05	-0.35	-0.29	<b>1.16</b>
Imax	0.8cap	0.01	-1.62	-0.19	-0.13	<b>1.64</b>

Results taken from DIN variant 5-85A Report 137550 dated 24th September 2010

<b>SGS</b>	EC-Type Examination Certificate Number: <b>0120/ SGS0046</b>		
	Issue Number: 5		Dated: 17 <sup>th</sup> May 2012

In addition to the accuracy requirements the composite error  $e_c$  of the meter is shown below

The composite error at a certain load is calculated from the following formula:

$$e_c = \sqrt{e^2(I.\cos\theta) + e^2(T.I.\cos\theta) + e^2(U.I.\cos\theta) + e^2(f.I.\cos\theta)}$$

where

$e^2(I.\cos\theta)$	=	Intrinsic error of meter at a certain load
$e^2(T.I.\cos\theta)$	=	Additional error due to variation of the temperature at the same load
$e^2(U.I.\cos\theta)$	=	Additional error due to variation of the voltage at the same load
$e^2(f.I.\cos\theta)$	=	Additional error due to variation of the frequency at the same load

Ambient Temperature Range 5 to 30 Degrees C						
Current	PF Cos	e(Icos)	e(TIcos)	e(Uicos)	e(ficos)	%MPE
Imin	1.0	0.07	0.68	-0.09	0.07	<b>0.69</b>
Itr	1.0	0.31	0.81	0.08	0.09	<b>0.88</b>
10ltr	1.0	0.45	0.71	0.17	0.10	<b>0.86</b>
Imax	1.0	0.41	0.78	0.11	-0.09	<b>0.89</b>
Itr	0.5ind	0.24	0.67	0.08	-0.06	<b>0.72</b>
10ltr	0.5ind	0.45	0.72	-0.19	-0.09	<b>0.87</b>
Imax	0.5ind	0.43	0.65	-0.21	-0.10	<b>0.81</b>
Itr	0.8cap	0.23	0.71	0.03	0.02	<b>0.75</b>
10ltr	0.8cap	0.41	0.87	0.13	0.17	<b>0.99</b>
Imax	0.8cap	0.44	0.81	0.20	0.07	<b>0.95</b>

Ambient Temperature Range -10 to 40 Degrees C						
Current	PF Cos	e(Icos)	e(TIcos)	e(Uicos)	e(ficos)	%MPE
Imin	1.0	0.07	1.09	-0.09	0.07	<b>1.10</b>
Itr	1.0	0.31	1.06	0.08	0.09	<b>1.11</b>
10ltr	1.0	0.45	1.00	0.17	0.10	<b>1.11</b>
Imax	1.0	0.41	0.95	0.11	-0.09	<b>1.04</b>
Itr	0.5ind	0.24	1.07	0.08	-0.06	<b>1.10</b>
10ltr	0.5ind	0.45	0.82	-0.19	-0.09	<b>0.96</b>
Imax	0.5ind	0.43	0.96	-0.21	-0.10	<b>1.08</b>
Itr	0.8cap	0.23	1.03	0.03	0.02	<b>1.06</b>
10ltr	0.8cap	0.41	1.03	0.13	0.17	<b>1.13</b>
Imax	0.8cap	0.44	1.00	0.20	0.07	<b>1.11</b>

<b>SGS</b>	EC-Type Examination Certificate Number:					
	<b>0120/ SGS0046</b>					
	Issue Number: 5				Dated: 17 <sup>th</sup> May 2012	

Ambient Temperature Range -25 to 55 Degrees C						
Current	PF Cos	e(Icos)	e(TIcos)	e(Uicos)	e(fIcos)	%MPE
Imin	1.0	0.07	1.24	-0.09	0.07	<b>1.25</b>
Itr	1.0	0.31	1.29	0.08	0.09	<b>1.33</b>
10ltr	1.0	0.45	1.31	0.17	0.10	<b>1.40</b>
Imax	1.0	0.41	1.26	0.11	-0.09	<b>1.33</b>
Itr	0.5ind	0.24	1.19	0.08	-0.06	<b>1.22</b>
10ltr	0.5ind	0.45	1.12	-0.19	-0.09	<b>1.23</b>
Imax	0.5ind	0.43	1.12	-0.21	-0.10	<b>1.22</b>
Itr	0.8cap	0.23	1.31	0.03	0.02	<b>1.33</b>
10ltr	0.8cap	0.41	1.31	0.13	0.17	<b>1.39</b>
Imax	0.8cap	0.44	1.30	0.20	0.07	<b>1.39</b>

Results taken from BS variant 5-100A Report 150370 dated 17th August 2011137550

	<b>EC-Type Examination Certificate Number:</b> <b>0120/ SGS0046</b>	
Issue Number: 5		Dated: 17 <sup>th</sup> May 2012

#### 4. Annex of Variants

Product Variant Identification Details:

Type Designation	Description of meter															
<b>U<sub>n</sub></b>	<b>I<sub>b</sub></b>	<b>I<sub>max</sub></b>	<b>SINGLE PHASE (A100C) MODEL CODE</b>													
			<b>TYPE</b>													
<b>PRODUCT/TERMINATION</b>	<b>S</b>	<b>J</b>	<b>1</b>	<b>L</b>	<b>A</b>	<b>B</b>	<b>E</b>	<b>S</b>	<b>S</b>	<b>G</b>	<b>N</b>	<b>S</b>	<b>J</b>	<b>-</b>	<b>C</b>	<b>F</b>
Single Phase, BS terminal arrangement (L-N-N-L)	S	J	1	L	A	B	E	S	S	G	N	S	J	-	C	F
Single Phase, DIN terminal arrangement (L-L-N-N)	S	K														
<b>SERVICE TYPE</b>																
1-phase 2-wire																
<b>CURRENT RANGE</b>																
10-60A DIN or BS (Imax any integral of Ib up to 60A, or 65A)																D
5-60A DIN or BS (Imax any integral of Ib up to 60A, or 65A)																F
20-100A BS only (Imax any integral of Ib up to 100A)																L
10-100A BS only (Imax any integral of Ib up to 100A)																M
5-100A BS only (Imax any integral of Ib up to 100A)																N
5-85A DIN only (Imax any integral of Ib up to 85A)																P
<b>VOLTAGE</b>																
220 - 250V																A
<b>FREQUENCY, ACCURACY CLASS</b>																
50 Hz, Class 1 kWh (IEC62053-21) – see note 1, Cl.B kWh,(EN 50470-3)																B
50 Hz, Class 2 kWh (IEC62053-21) – see note 1 Cl.A kWh,(EN 50470-3)																C
<b>TARIFF &amp; HARDWARE CONFIGURATION</b>																
Single Rate, kWh registration																B
Two-rate, kWh registration, switched to neutral																E
<b>DISPLAY CONFIGURATION</b>																
Customer specified display configuration																S
<b>DISPLAY CYCLE, REGISTER SOURCES</b>																
Customer specified display sequence and register sources																S
<b>TEST INDICATOR(S) (see important note 3)</b>																
Non-modulated 40ms pulses																G
<b>PULSING/ABSOLUTE OUTPUT(see important note 3 overleaf)</b>																
No pulse or serial data output																N
SO pulse output, tied to neutral, one auxiliary terminal (2-rate only)																P
SO pulse output, floating, two auxiliary terminals (1-rate only)																Q
Absolute serial data output - tied to neutral, one auxiliary terminal (2-rate only, not with 1107)																S
Absolute serial data output - floating, two auxiliary terminals (1-rate only, not with 1107)																T
<b>COMMUNICATIONS</b>																
IrDA optical port, data rate set at time of manufacture																S
<b>OTHER OPTIONS</b>																
Extended BS terminal cover, with cut-out for cables, slotted brass main terminal screws																B
Extended BS terminal cover no cut-out for cables, "Israel" sealing boss, slotted brass main terminal screws																H
DIN: extended terminal cover no cut-out for cables. BS: non-extended terminal cover																J
DIN: short terminal cover. BS: extended terminal cover, no cut-out for cables																K
Extended DIN terminal cover, with cut-out for cables																T
Extended BS terminal cover, with cut-out for cables																U
Clear short non-removing BS terminal cover, slotted brass large head main terminal screws																X
Clear short DIN terminal cover, slotted brass large head main terminal screws																Y
Supplied without terminal cover																Z
<b>VERSION</b>																
IrDA																- C
<b>SPECIAL ADDITIONS</b>																
Firmware 2-01167-F (IrDA) – BS version and DIN version IEC and MID approved																F

<b>SGS</b>	EC-Type Examination Certificate Number:	
	<b>0120/ SGS0046</b>	
	Issue Number: 5	Dated: 17 <sup>th</sup> May 2012

Modifications to the meter(s) described according to approval No.**0120/ SGS0046** must be notified to the issuing body to confirm the meter(s) continuing compliance to the relevant pattern approval standard(s).

## 5. Document Revision History

Issue	Date	Comments
1	30/10/2009	Initial Issue
2	24/09/2010	Additional approval of DIN Terminal only 0,25-5(85)A Current Range
3	17/08/2011	Additional approval of BS Terminal 0,25-5(100)A Current Range
4	31/08/2011	Corrected product variant annex
5	17/05/2012	Migration to new MID certificate template